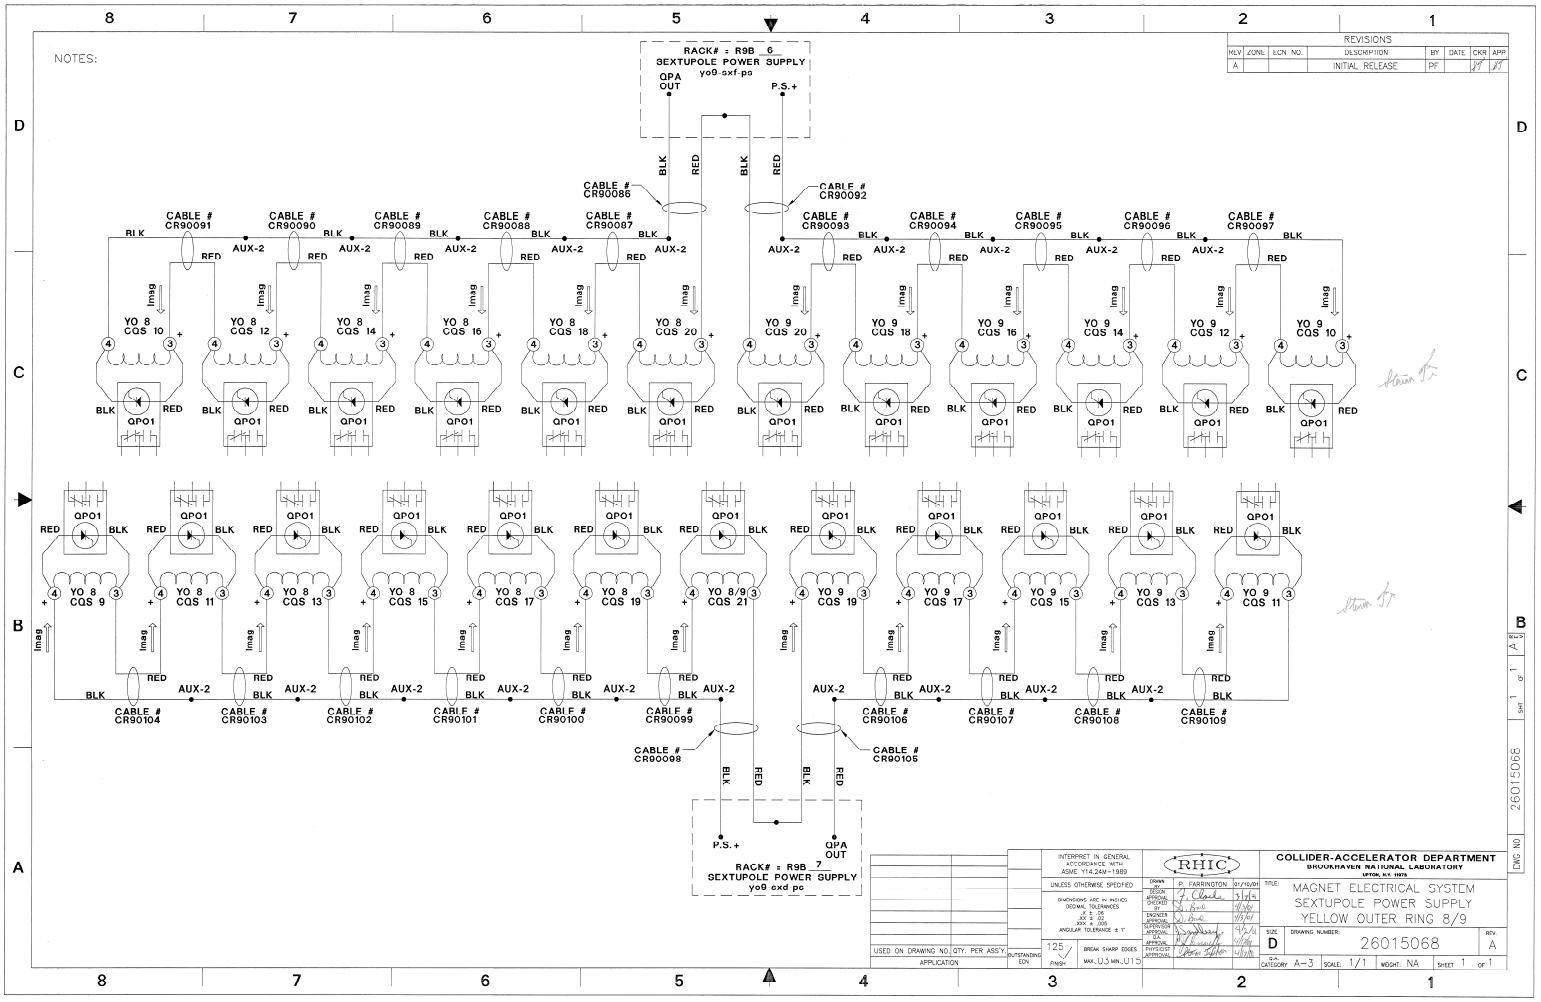
NOTES:
RACK# : R9B 6
SEXTUPOLE POWER SUPPLY
yo9-sxf-ps
QPA OUT
P.S.+
CABLE # CR90086
CABLE # CR90092
CABLE # CR90091
CABLE # CR90090
CABLE # CR90089
CABLE # CR90088
CABLE # CR90087
CABLE # CR90093
CABLE # CR90094
CABLE # CR90095
CABLE # CR90096
CABLE # CR90097
YO 8 CQS 10
YO 8 CQS 12
YO 8 CQS 14
YO 8 CQS 16
YO 8 CQS 18
YO 8 CQS 20
YO 9 CQS 20
YO 9 CQS 18
YO 9 CQS 16
YO 9 CQS 14
YO 9 CQS 12
YO 9 CQS 10
YO 8 CQS 9
YO 8 CQS 11
YO 8 CQS 13
YO 8 CQS 15
YO 8 CQS 17
YO 8 CQS 19
YO 8/9 CQS 21
YO 9 CQS 19
YO 9 CQS 17
YO 9 CQS 15
YO 9 CQS 13
YO 9 CQS 11
CABLE # CR90104
CABLE # CR90103
CABLE # CR90102
CABLE # CR90101
CABLE # CR90100
CABLE # CR90099
CABLE # CR90106
CABLE # CR90107
CABLE # CR90108
CABLE # CR90109
CABLE # CR90098
CABLE # CR90105
RACK# : R9B 7
SEXTUPOLE POWER SUPPLY
yo9 cxd pc
BLK
RED
AUX-2
Imag
QPO1
REVISIONS
REV | ZONE | ECN NO. | DESCRIPTION | BY | DATE | CKR | APP
A | | | INITIAL RELEASE | PF | | | |
INTERPRET IN GENERAL ACCORDANCE WITH ASME Y14.24M-1989
UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES
DECIMAL TOLERANCES
.X ± .05
.XX ± .02
.XXX ± .005
ANGULAR TOLERANCE ± 1°
USED ON DRAWING NO. | QTY. PER ASS'Y.
APPLICATION
OUTSTANDING EDN
125 / FINISH
BREAK SHARP EDGES
MAX. .03 MIN. .015
RHIC
DRAWN BY P. FARRINGTON 01/10/01
DESIGN APPROVAL
CHECKED BY
ENGINEER APPROVAL
SUPERVISOR APPROVAL
APPROVAL
PHYSICIST APPROVAL
COLLIDER-ACCELERATOR DEPARTMENT
BROOKHAVEN NATIONAL LABORATORY
UPTON, N.Y. 11973
TITLE: MAGNET ELECTRICAL SYSTEM
SEXTUPOLE POWER SUPPLY
YELLOW OUTER RING 8/9
SIZE D
DRAWING NUMBER: 26015068
REV. A
Q.A. CATEGORY A-3
SCALE: 1/1
WEIGHT: NA
SHEET 1 OF 1
DWG NO 26015068
SHT 1 OF 1
REV A